

Figure 1 - Comparison of control line signal at 40 and 60 sec for nitrocellulose of different flow rates using 0 mIU/mL hCG urine standard

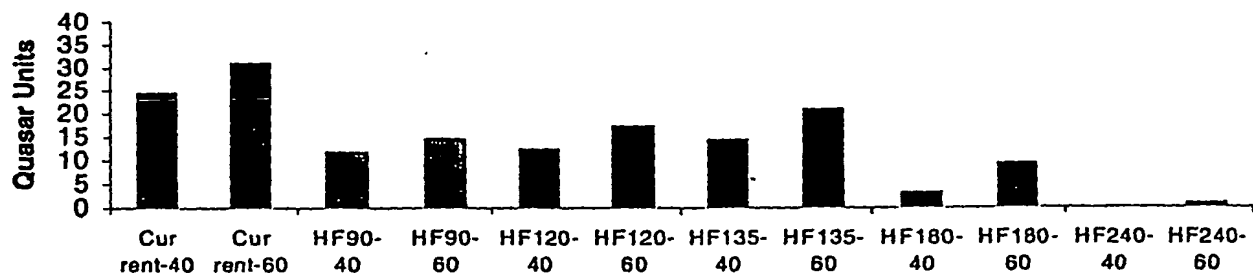


Figure 2 - Comparison of control line signal at 40 and 60 sec for nitrocellulose of different flow rates using 400 mIU/mL hCG urine standard

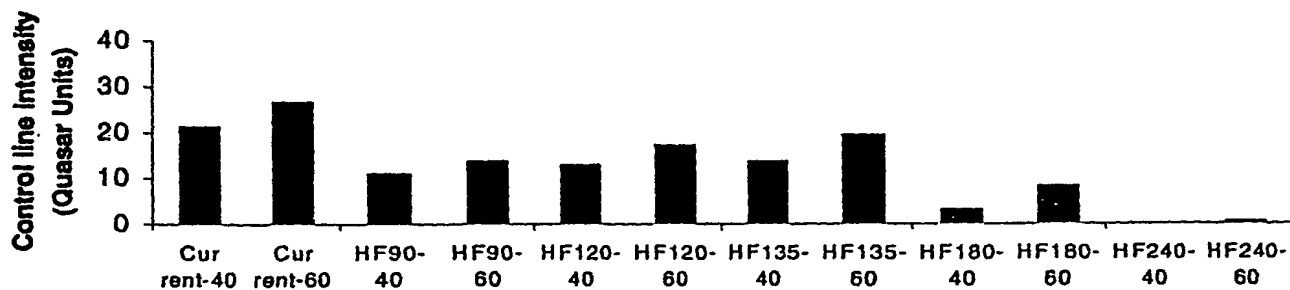


Figure 3

